

Aberystwyth University

Spatially resolved infrared radiofluorescence: single-grain K-feldspar dating using CCD imaging

Mittelstraß, Dirk; Kreuzer, Sebastian

Published in:
Geochronology

DOI:
[10.5194/gchron-3-299-2021](https://doi.org/10.5194/gchron-3-299-2021)

Publication date:
2021

Citation for published version (APA):

Mittelstraß, D., & Kreuzer, S. (2021). Spatially resolved infrared radiofluorescence: single-grain K-feldspar dating using CCD imaging. *Geochronology*, 3(1), 299-319. <https://doi.org/10.5194/gchron-3-299-2021>

Document License CC BY

General rights

Copyright and moral rights for the publications made accessible in the Aberystwyth Research Portal (the Institutional Repository) are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the Aberystwyth Research Portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the Aberystwyth Research Portal

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

tel: +44 1970 62 2400
email: is@aber.ac.uk



Supplement of

Spatially resolved infrared radiofluorescence: single-grain K-feldspar dating using CCD imaging

Dirk Mittelstraß and Sebastian Kreutzer

Correspondence to: Dirk Mittelstraß (dirk.mittelstrass@luminescence.de) and Sebastian Kreutzer (sebastian.kreutzer@aber.ac.uk)

The copyright of individual parts of the supplement might differ from the article licence.

1 Additional figures

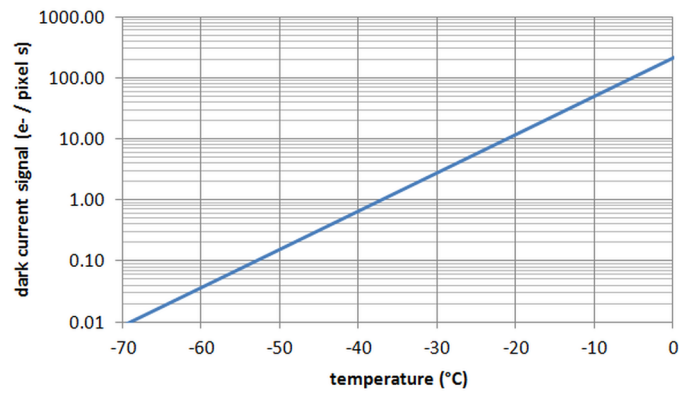


Figure S1: Approximated dependency of the dark current on the chip temperature of the EM-CCD camera.

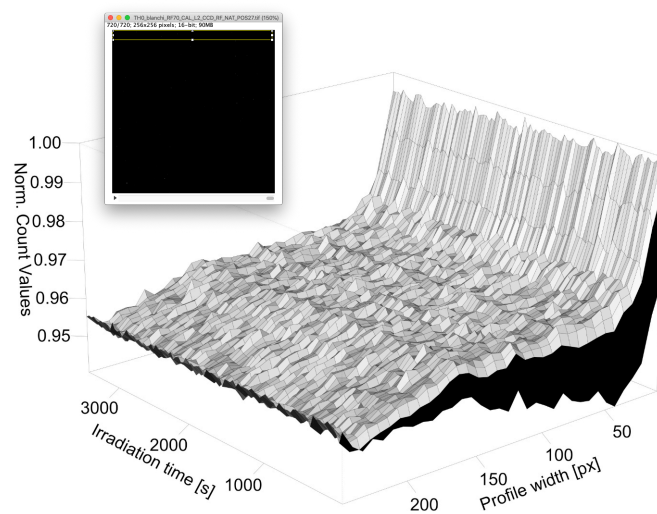


Figure S2: Normalised IR-RF background recorded over 3,600 s. The background profile is the sum signal of the rectangle pixel selection shown in the inset. The background signal noise is not homogeneous over the chip surface, indicating a problem with the cooling or sealing of the optics from external stray light. However, over the recorded 3,600 s, the signal decay is around 0.05% and considered stable.

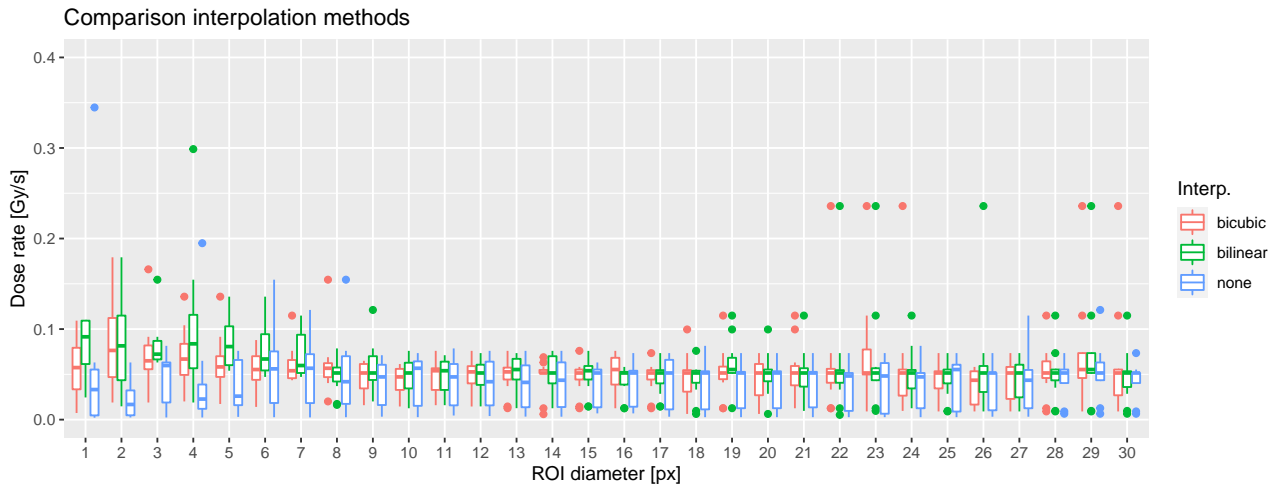


Figure S3: The figure shows boxplots of the source dose rate measured with the sample TH0 for three different signal interpolation types used for the image alignment. The bicubic interpolation seems to provide the most stable results, while no interpolation leads to a significant scatter and unrealistic dose rate results.

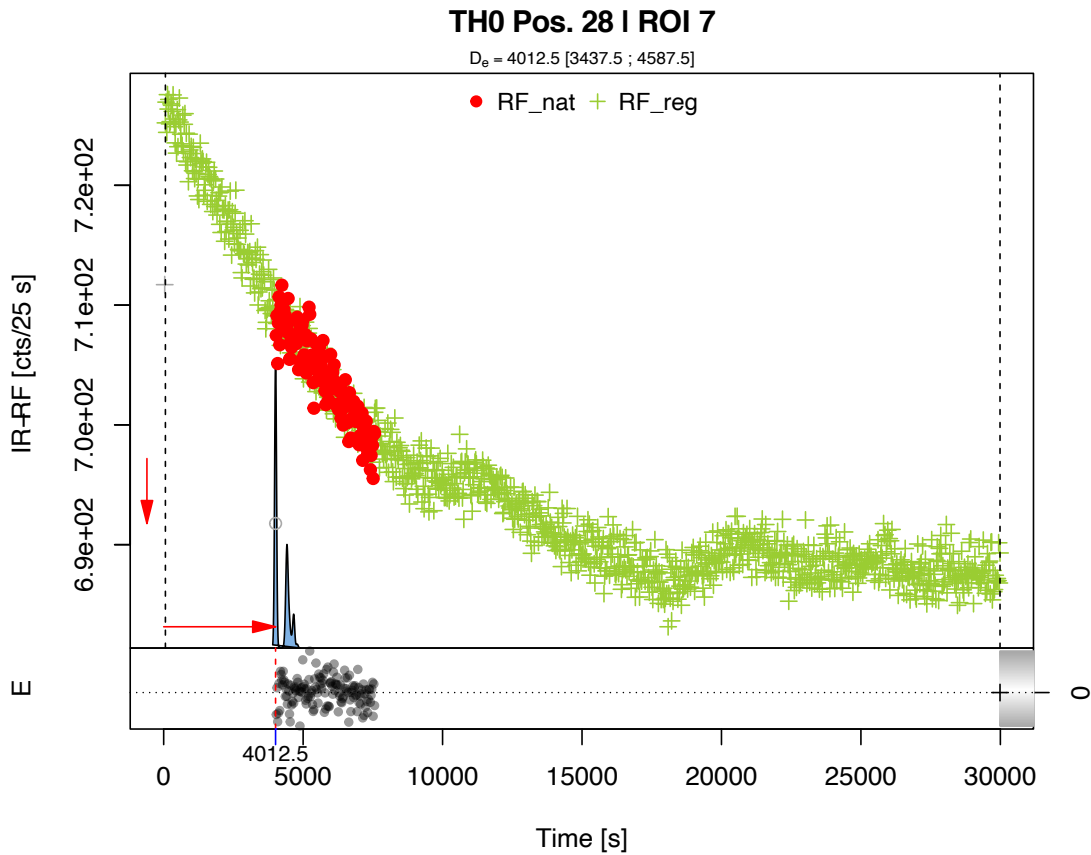


Figure S4: Example of an IR-RF curve extracted from an image (here ROI 7, cup on pos 28 on the sample carousel) of sample TH0. Due to the cooling system's degradation, the background signal varied considerably, rendering the measured curves unusable for further analysis.

TH0 (PMT)

n = 10 | average = 0.0564 | SE(average) = 0.0012

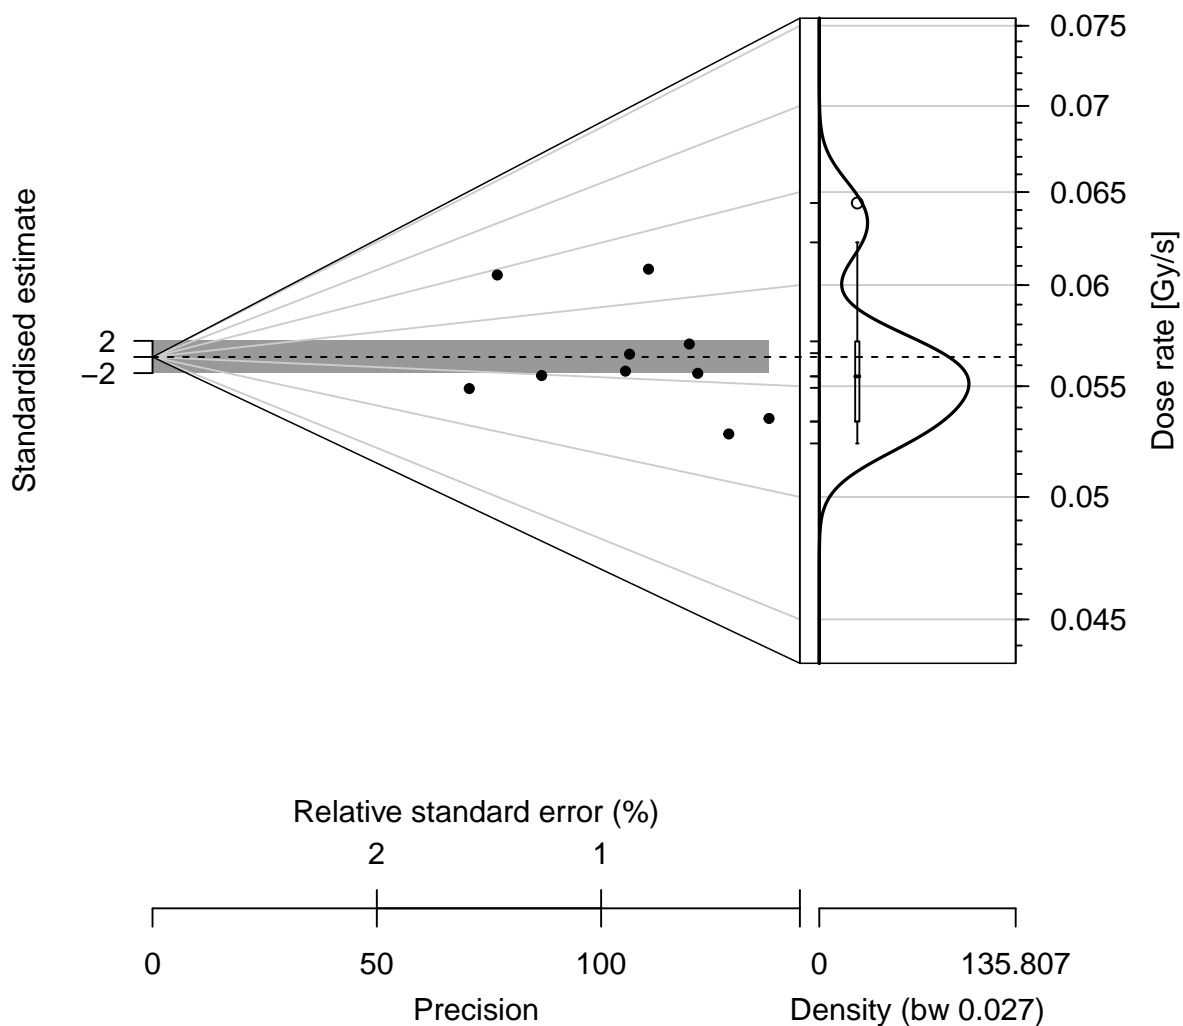


Figure S5: TH0 IR-RF measurement results. The IR-RF curves were measured with the PMT; in total, ten aliquots. The average dose was calculated with the average dose model. SE indicates the standard error as returned by the average dose model. Further details see the manuscript.